
Sabina II

#### **Quick Reference Guide**

English

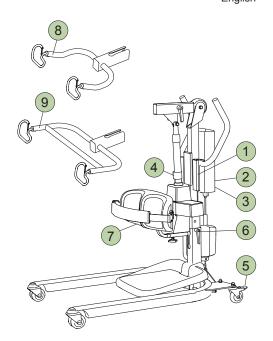


#### Safety Instructions

- Read the instruction guides for the lift and lifting accessories before use.
- Plan the lifting operation carefully.
- Check to ensure that the sling's strap loops are correctly connected to the sling bar hooks when the sling strap is extended, but before the patient is lifted from the underlying surface.
- Maximum load active lifting: 200 kg (440 lbs) Maximum load passive lifting: 150 kg (330 lbs)


To retain max. load it is essential to use accessories rated for the same max. load or greater.

#### **IMPORTANT!**


This quick reference guide does not replace the lift's instruction guide, which can be downloaded at www.liko.com.

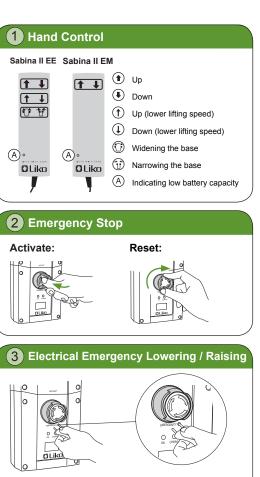

 $\Delta$  The object used to press must not be sharp, since this may cause damage on the control box!



# 5 Locking the Wheels



#### Alternative Use





Charge immediately!

# Charging the Batteries



Fully charged

- Charge the lift regularly after use.
- The lift does not function during charging.
- The emergency stop should not be pressed in during charging.

#### Ergonomics

- Never lift manually let the lift do the lifting.
- Take it easy. Work calmly and methodically.
- Don't strain your back! Work in a walking stance with your back straight.
- Reduce the lever effect. Work close to the patient and the lift.

### Cleaning

When necessary, clean the lift with a moist cloth, using common surface cleaners or disinfectants.

### Simple Troubleshooting

#### Check to ensure that:

- the emergency stop is not pressed in, see (2)
- · the battery is charged
- the hand control is properly connected.

# Other Quick Reference Guides

Quick reference guides for Liko's lifts and slings are available for downloading at www.liko.com.

© Copyright Liko AB









www.liko.com

Manufacturer:

Liko AB Nedre vägen 100 SE-975 92 Luleå Sweden info@liko.se